

<p>المجلس الاعلى للمستشفيات الجامعية</p> <p>Proficiency Testing Unit</p> <p>Reference laboratory for Egyptian University Hospitals</p>	<p>Proficiency Testing</p>  <p>RLEUH PTU</p>  <p>EGAC Accredited</p>
--	--


Date: 30/01/2023

Dear Esteemed Colleague

Director of Microbiology Laboratory, TBI

Congratulations Your laboratory (Code: RL12) showed excellent performance with score 100% in MLA-04-2022 Program A. Attached full detailed report Wish you the best and sustainability of excellent laboratory service. keep on

Lab Code	ML-04a	ML-04b	ML-04c	ML-04d	ML-04e	ML-04 Overall
Score	20	20	20	20	20	100
RL12	20	20	20	20	20	100%

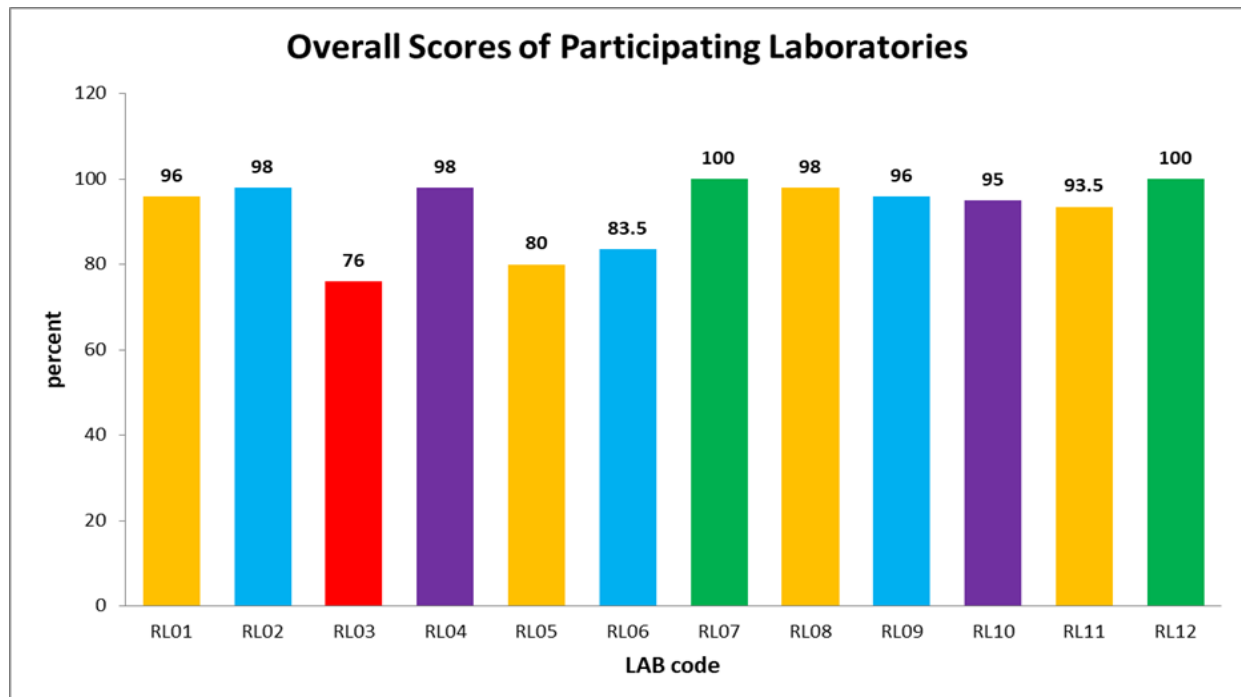

Best regards

PT Unit Director

Ghada /smail